

**A**

M 1 2 3 4 5 6 7 8 9 10

(bp)

1000 ←

700 ←

400 ←

300 ←

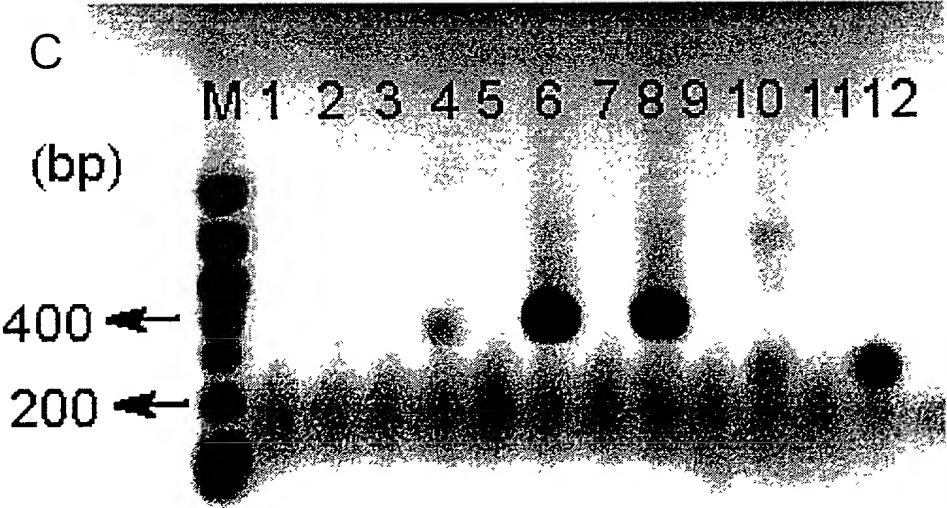
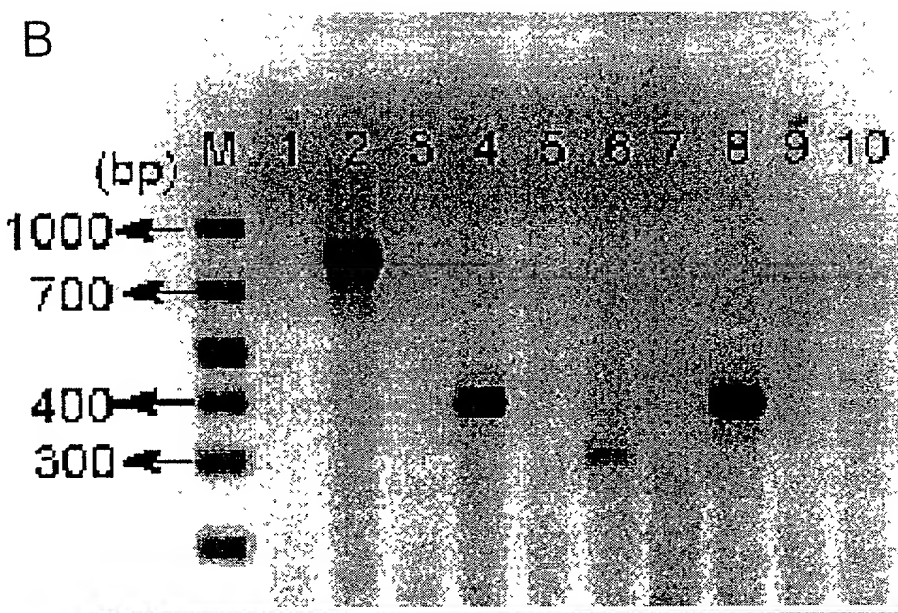


Fig 2

A

B

C

D

E



0.5 μm

Figure 3A

## Adhesive-Removal Test

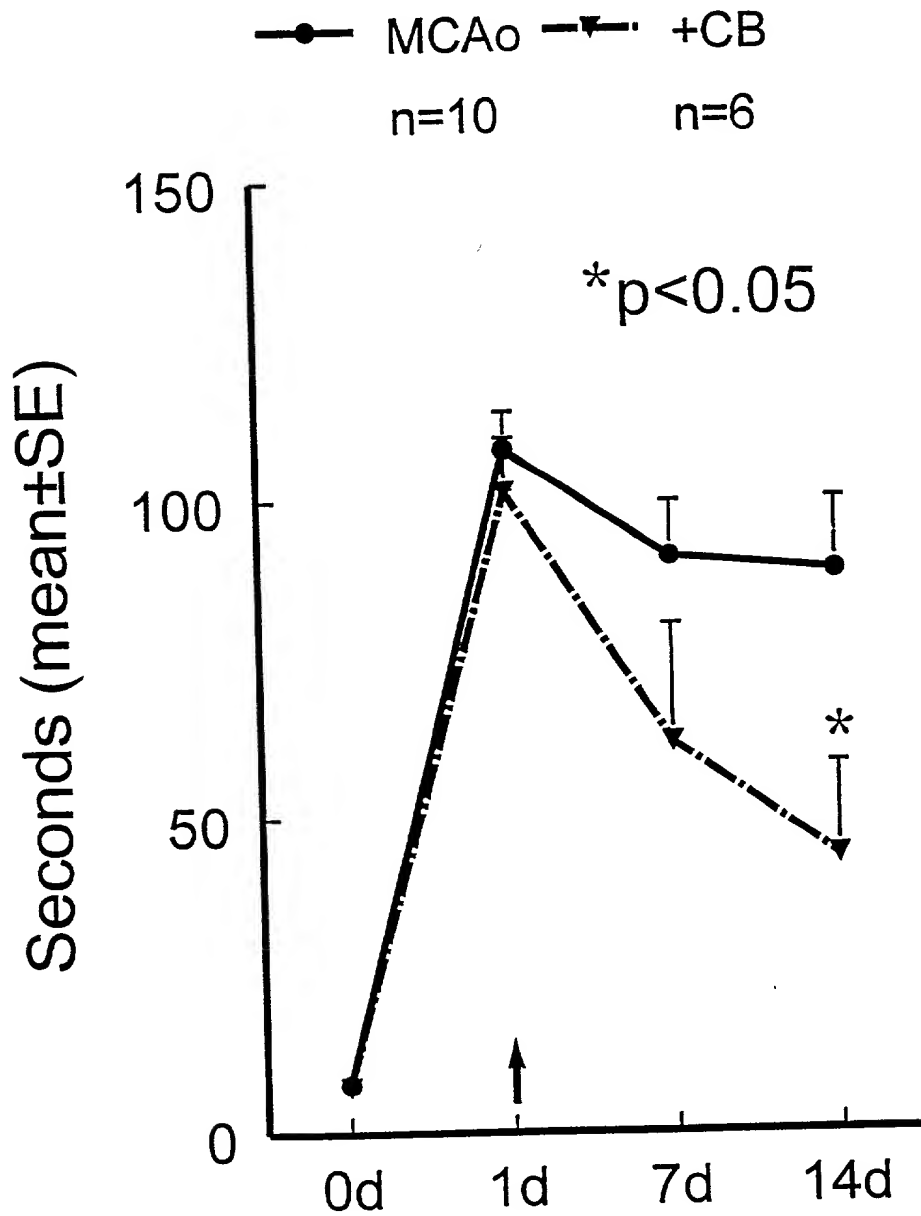


Figure 3B

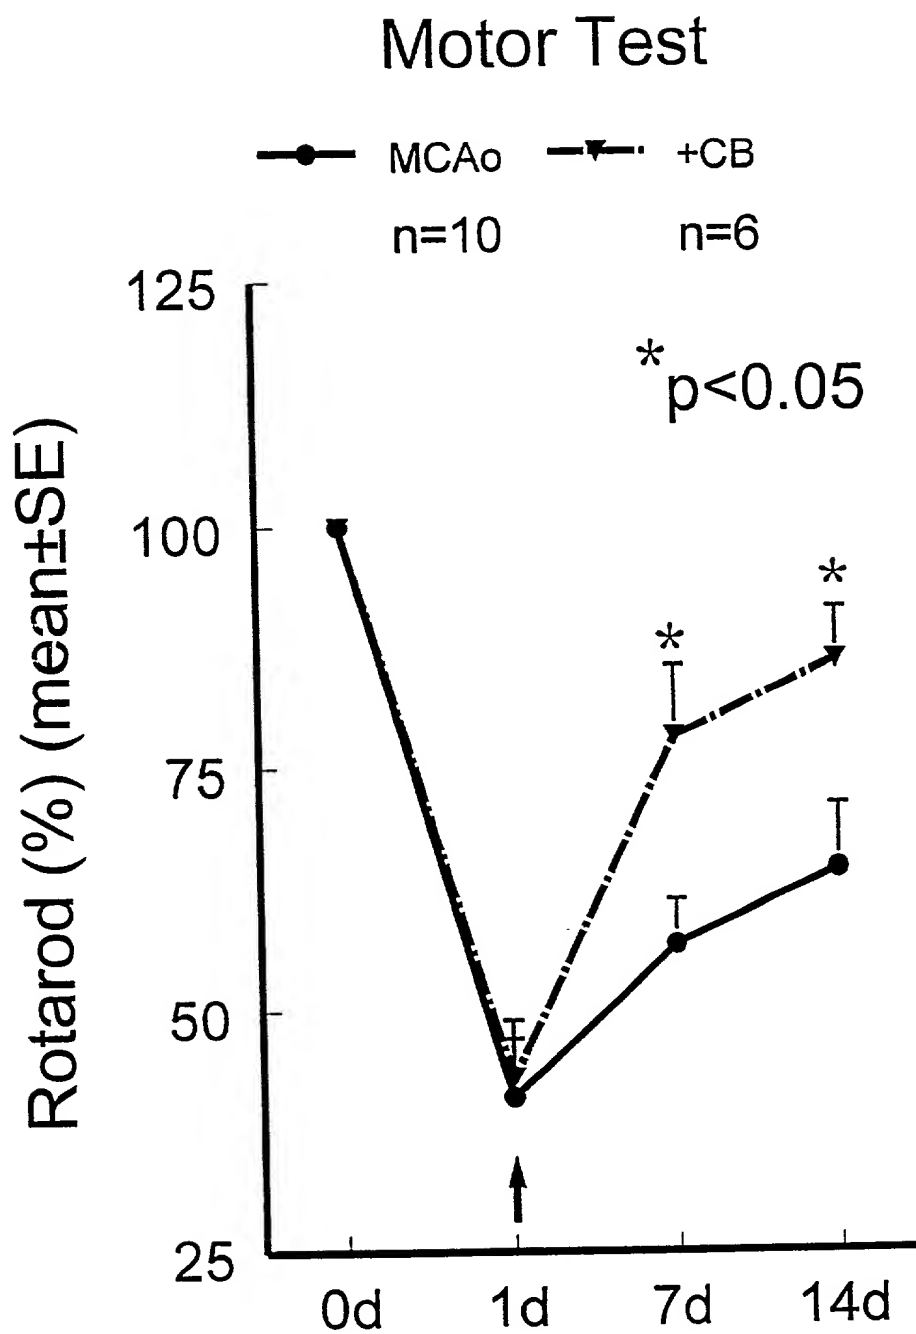


Figure 3C

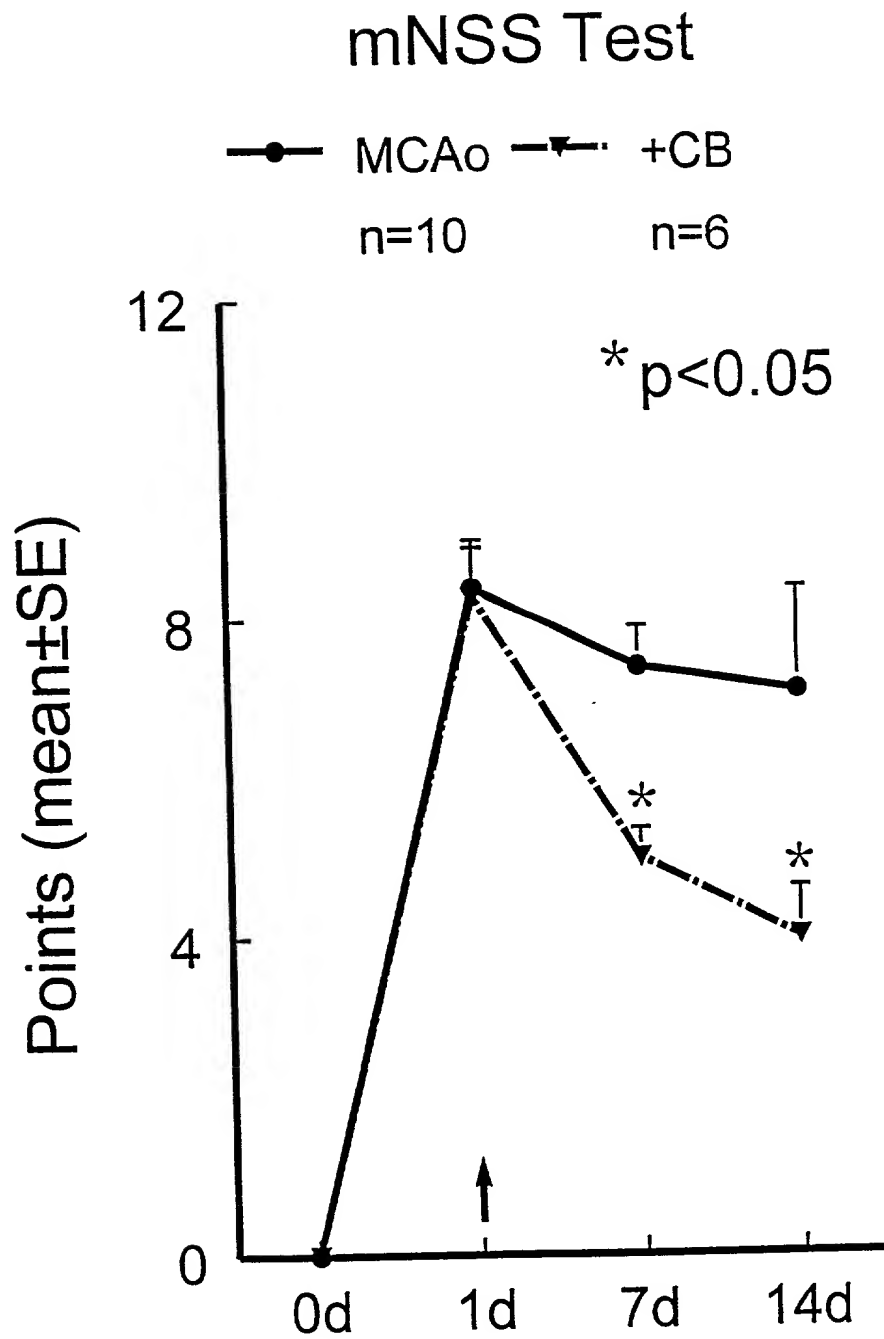


Figure 4A

## Adhesive-Removal Test

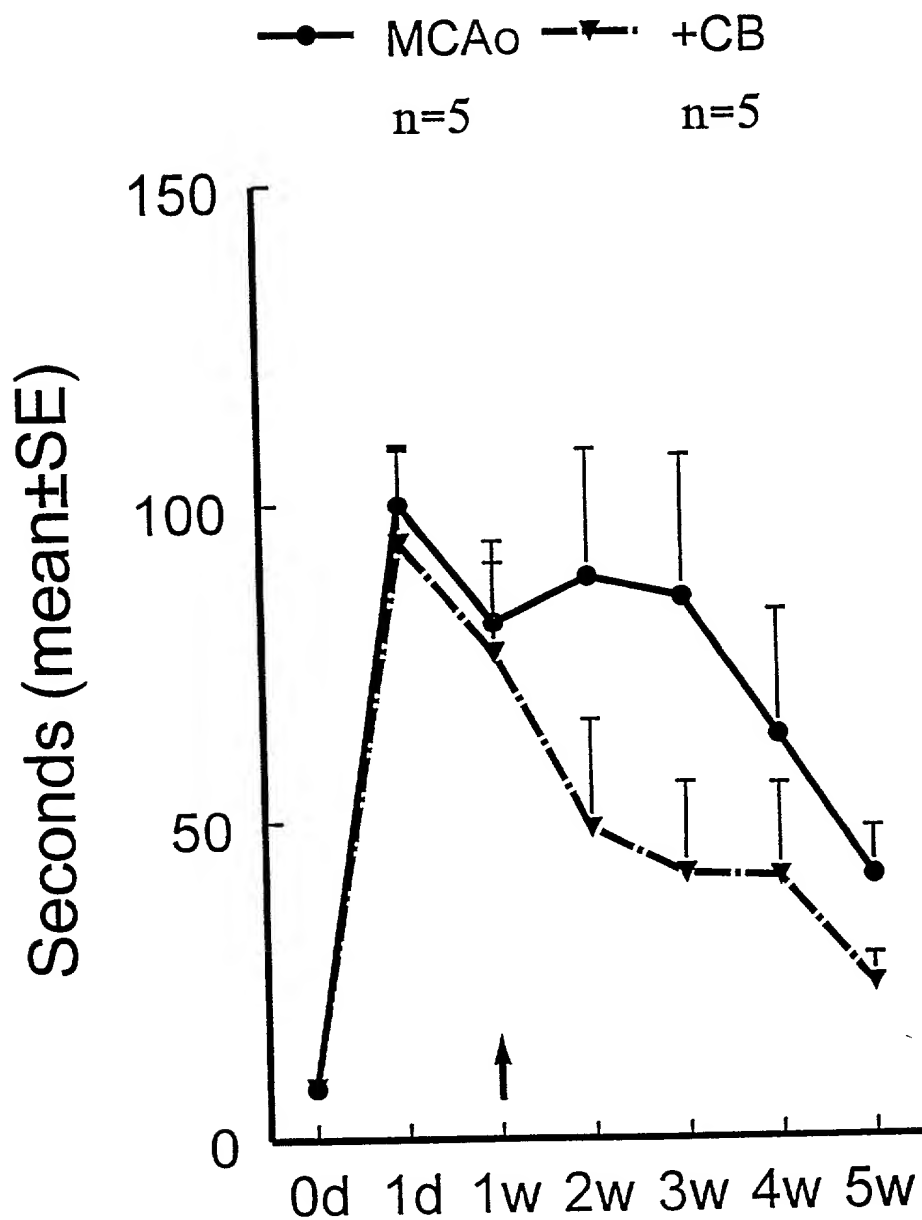


Figure 4B

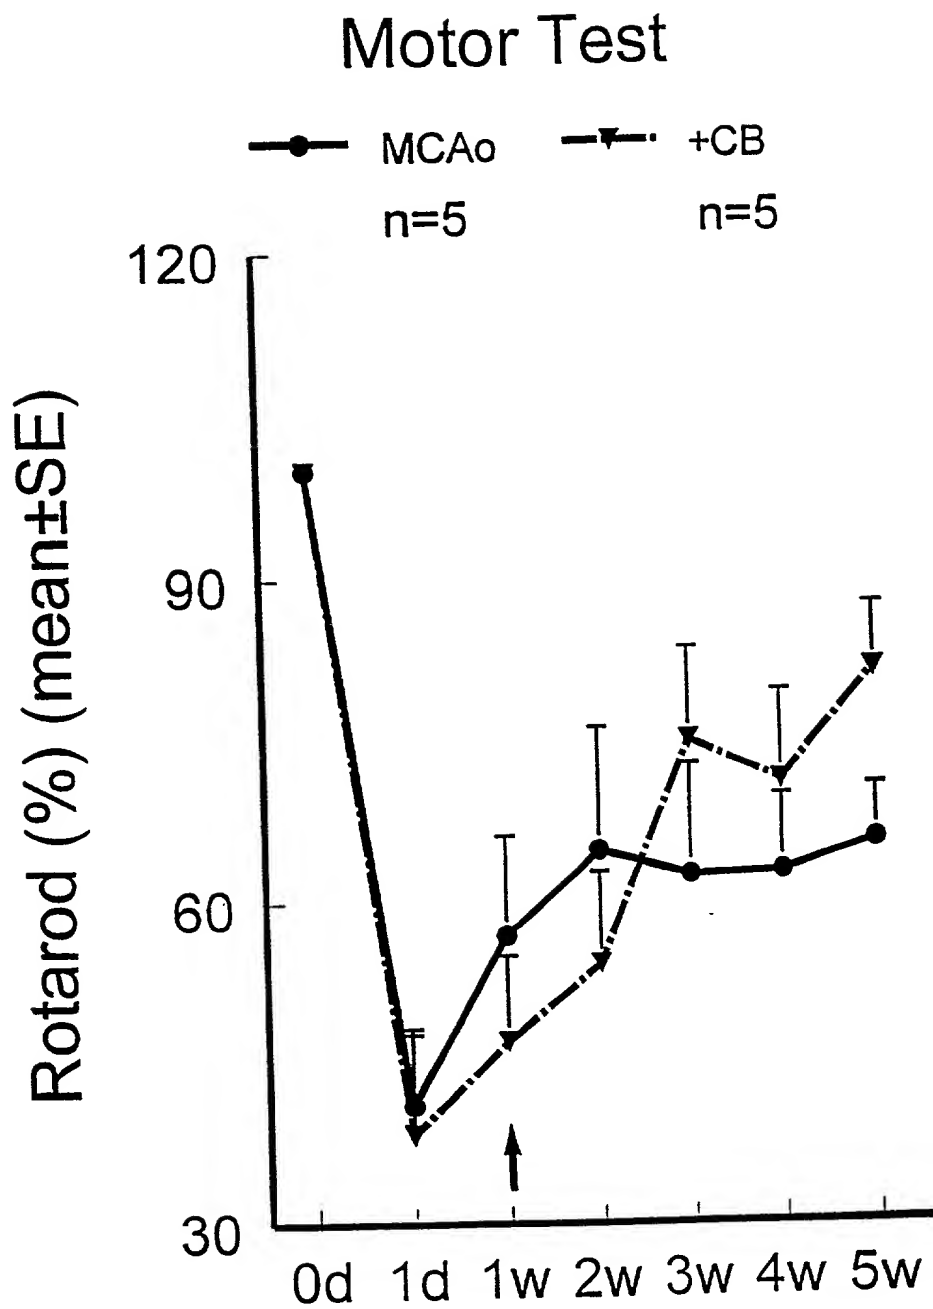


Figure 4C

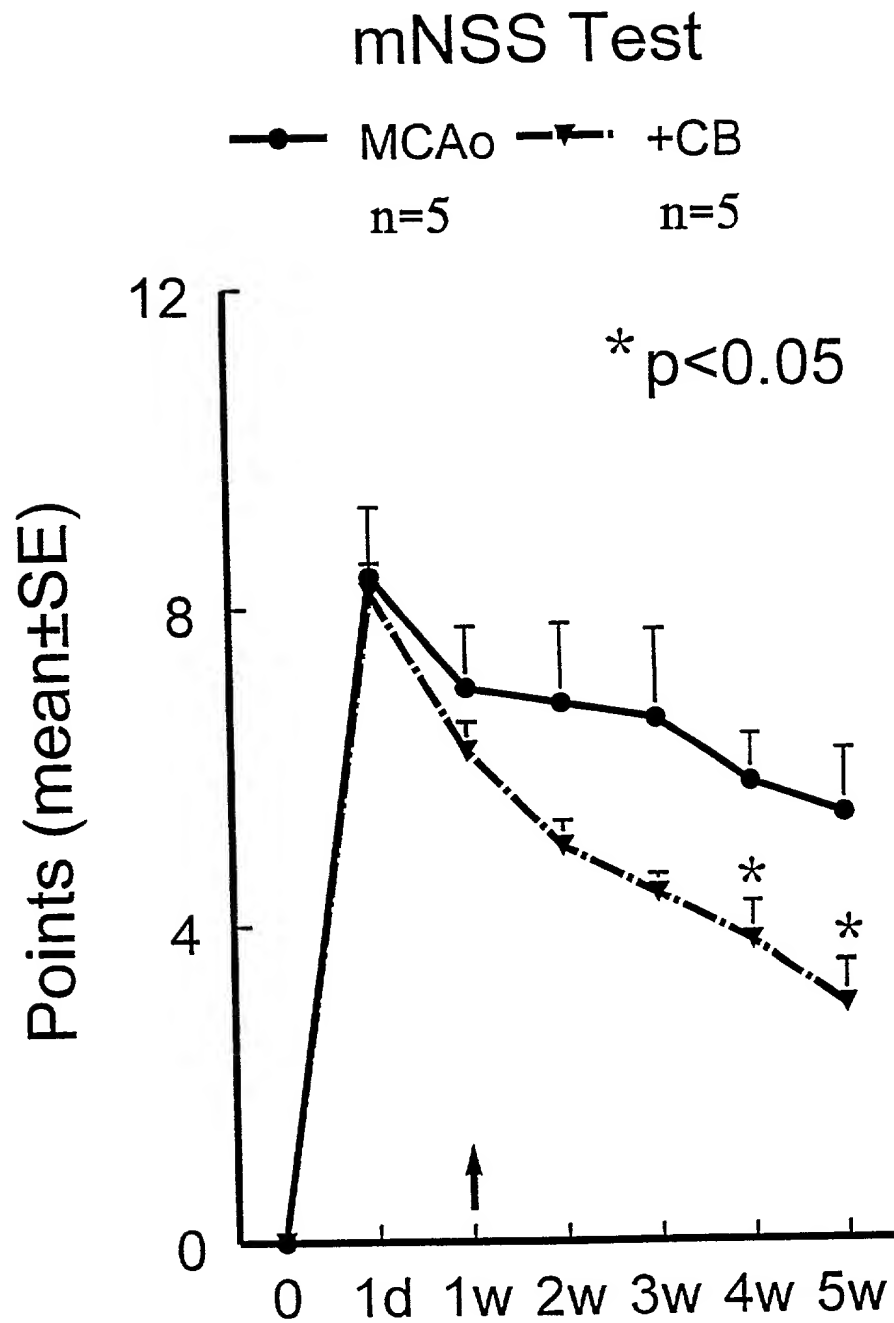




Figure 5

# Chemotaxis Assay-cord blood in vitro

